LABOMED®

PRIMA ENT
User Manual

Operating Surgical Microscopy

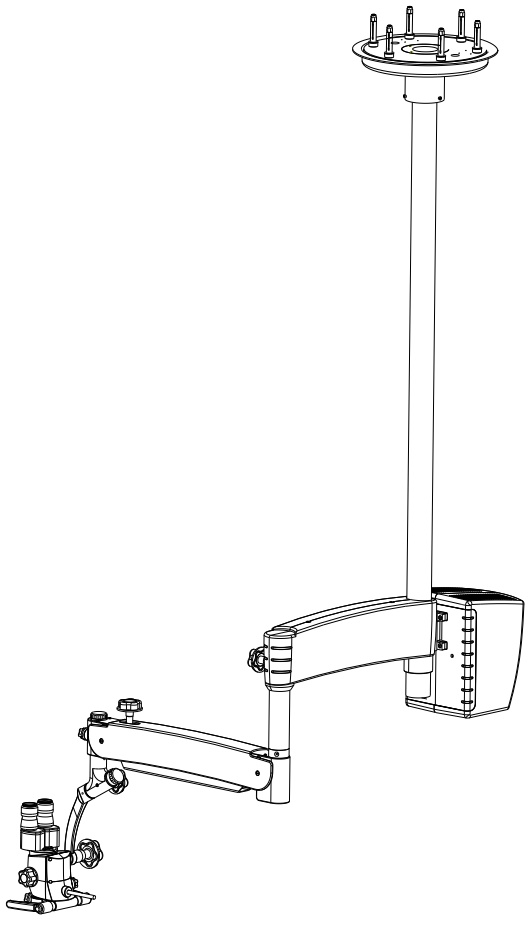

To ensure proper use of this instrument as well as to avoid injury while operating instrument, understanding this manual completely before use is highly recommended.

Ceiling mount for Prima DNT

Dimensions of ceiling mount used in dentistry

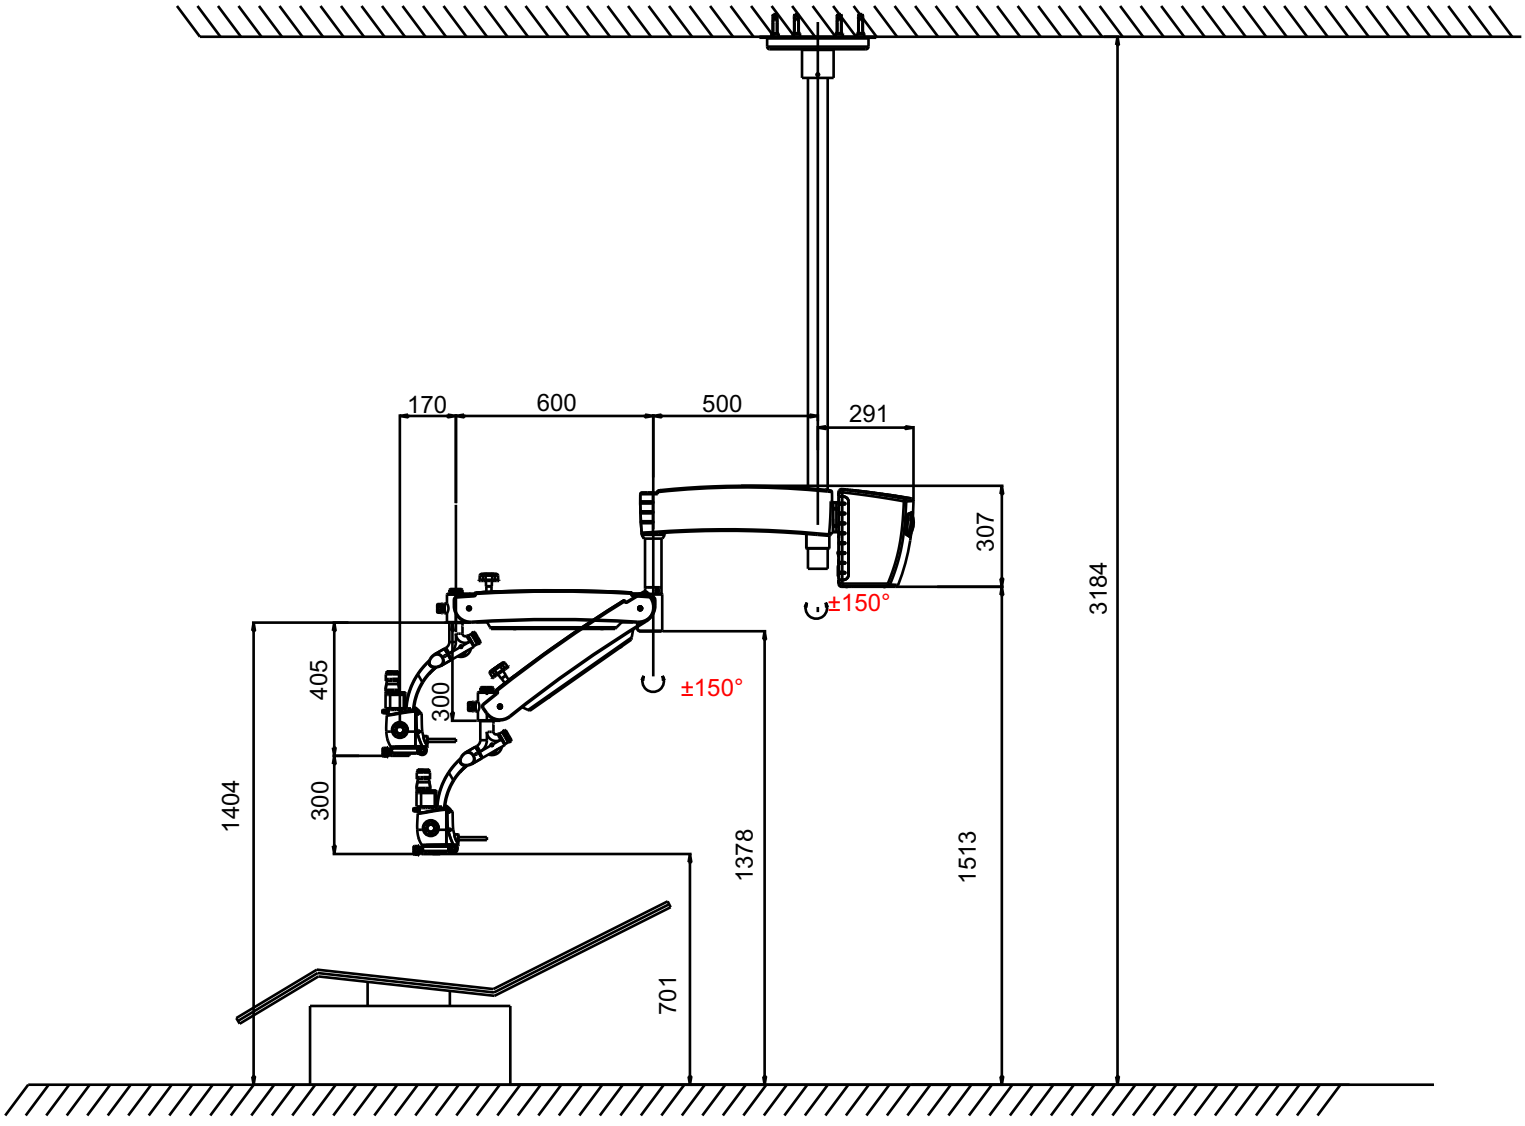

Ceiling mount: alternative installation to the patient’s side

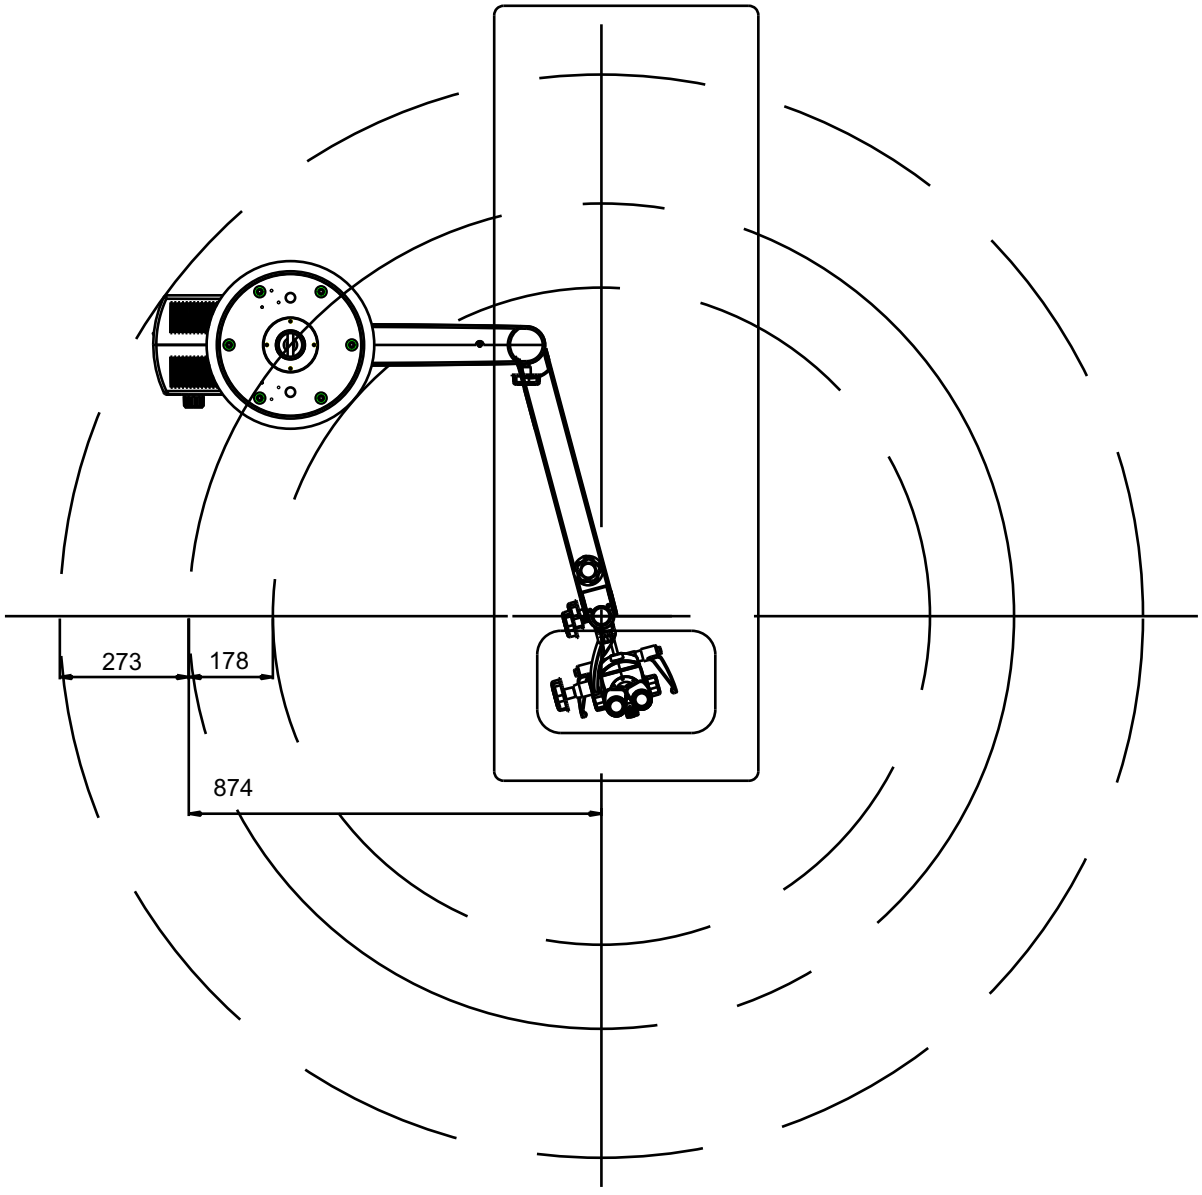

Ceiling mount for dentistry, recommended work ranges

Work range recommended for ideal installation site

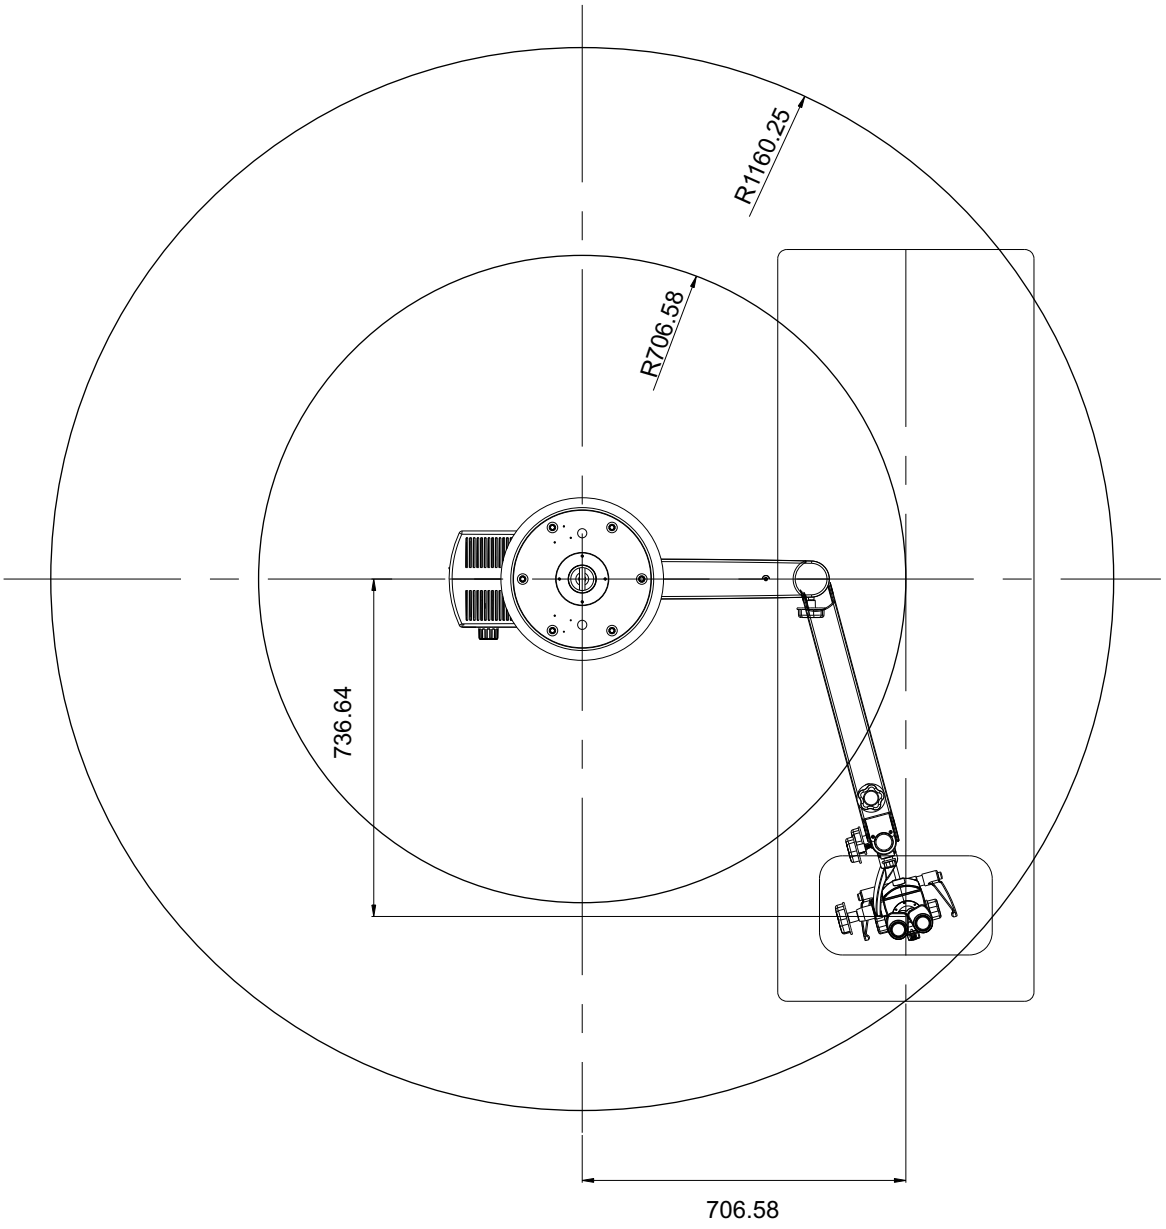

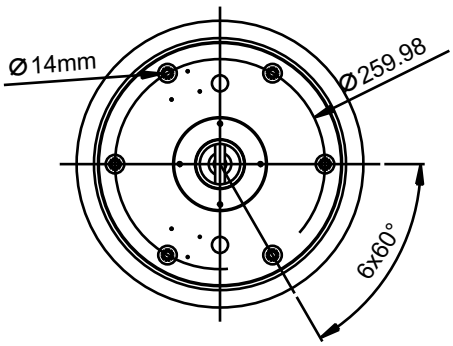
Ø14mm
Ø259.98
6x60°

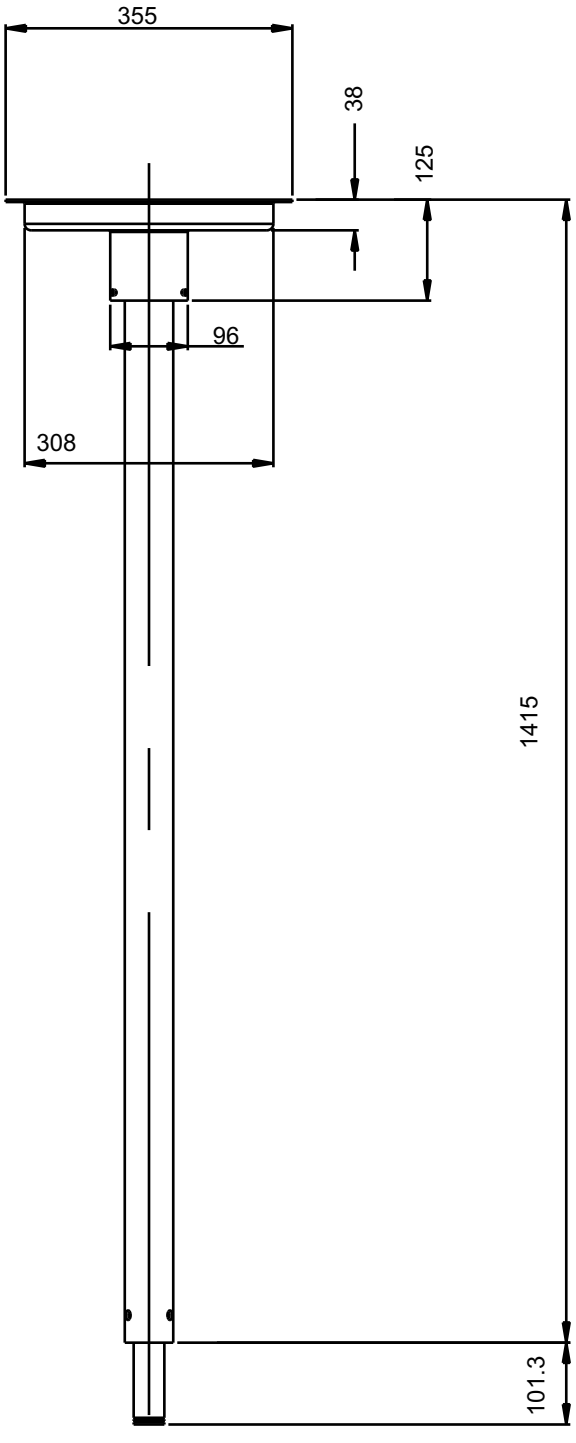
355
38
125
96
308
1415
101.3

www.laboamerica.com

Our policy is one of continuous development. Labo America, Inc., reserves the right to change design and specifications without prior notice.

Labo America Inc.
920 Auburn Court
Fremont
CA 94538

U.S.A.
Telephone: 510 445 1257
Fax: 510 991 9862
sales@laboamerica.com

LABOMED and Prima are registered trademarks of Labo America, Inc.
With a policy of continuous development, Labo America, Inc. reserves the right to change design and specifications without prior notice.

© 2010 Labo America, Inc.

ISO 9001 : 2008
File No. A9020

Printed in U.S.A.